

Propoxyphene (PPX) Rapid Test Kit (Colloidal Gold)

Product Name

Propoxyphene (PPX) Rapid Test Kit (Colloidal Gold)

Intended Use

Adopting highly specific antibody-antigen reaction and immunochromatographic technique, the test kit is used for qualitative detection of propoxyphene in urine and is suitable for screening of propoxyphene abuse.

Test Principle

The test kit adopts highly specific antibody-antigen reaction and immunochromatographic technique, and the kit contains propoxyphene antigen that is fixed on test area (T) of the membrane beforehand and colloidal gold marked anti- propoxyphene monoclonal antibody.

When testing, the urine chromatography up under the capillary effect. If the concentration of PPX in urine is lower than 300ng/ml, colloidal gold antibody can't combine with PPX completely. There will appear a purple strip in test area (T).If the concentration of PPX in urine is higher than 300ng/ml, colloidal gold combine with PPX completely, there will appear no purple strip in test area (T).During the testing process, because of lacking antibody-antigen reaction competitive reaction, there will appear a purple strip in test area (T).

Main Components

Sample pad, colloidal gold marked pad, nitrocellulose membrane, absorbent paper and PVC board.

Specimen requirement

1. Urine samples must be collected clean, dry and it does not contain any preservative glass containers. If a urine sample is visible turbidity form, must first centrifugal, filter or until the precipitation take clear liquid upper detection.
2. Samples should be used as soon as possible after being collected, it can't be placed at room temperature for a long time. If it can't be tested timely, it can be preserved for 3 days at 2-8℃,it need to be frozen at -20℃ for long-term preservation.

Storage and Expiry

Store at room temperature 4-30 ℃, avoid hot and sunshine, dry place, not frozen, valid for 24 months.

Test Procedure

Read the instruction carefully before testing. Beforehand, make the test kit and sample recovered to room temperature 15-30℃.The foil pouch can not be torn open until everything gets ready.

1. Open the foil pouch and take out the test strip/ cassette.
2. Test Procedure

2.1 Strip: Invade one end with an arrow of the strip into the container that filled with urine, take it out after 5s and put in on a clean and flat table. Note that the liquid level of urine can't excess the MAX line

of the test strip.

2.2 Cassette: Drop three drops (about 100uL) of urine sample in the sampling well with a pipette.

3. Read the test results within 5-10 minutes, it is invalid beyond 10 minutes.


Interpretation of Result

Positive: There only appear one purple strip in the control area (C), no purple strip appears in the test area (T).Positive result indicates: The concentration of PPX is higher than threshold value (300ng/mL).

Negative: There appear two purple strips, one is in test area (T) and the other is in control area(C).Negative result indicates: The concentration of PPX is lower than threshold value (300ng/mL).

Note: The color depth of purple strip in test area (T) may be different, within the prescribed observing period, regardless of the depth of the strip color, it should be judged as negative results in spite of a very weak purple strip.

Invalid: There is no purple strip in the control line(C), which indicates that incorrect operation or reagent failure, please re-test.

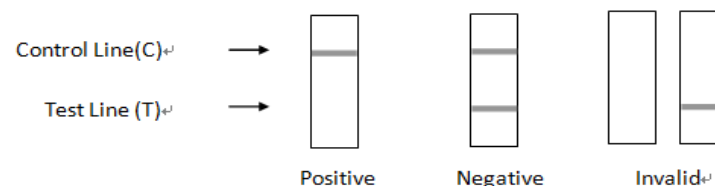

Limitations

1. This kit is only suitable for detection of reagent urine sample PPX.
2. The kit is for qualitative screening reagent, the content of PPX in urine can't be determined.
3. The kit is only used for screening, the negative result can't be used as basis for diagnosis.